


Nanodyne Replacement Illuminator for AO One-Ten Microscope: Included Items

Also Included but not shown:

- PN 10703 Hex Key 0.05 inch
- PN 10337 Hex Key 2mm Short Arm (for M3 BHCS)
- PN 11918 Hex Key 9/64 short arm

The illuminator should be powered by plugging the cable into the power supply provided.

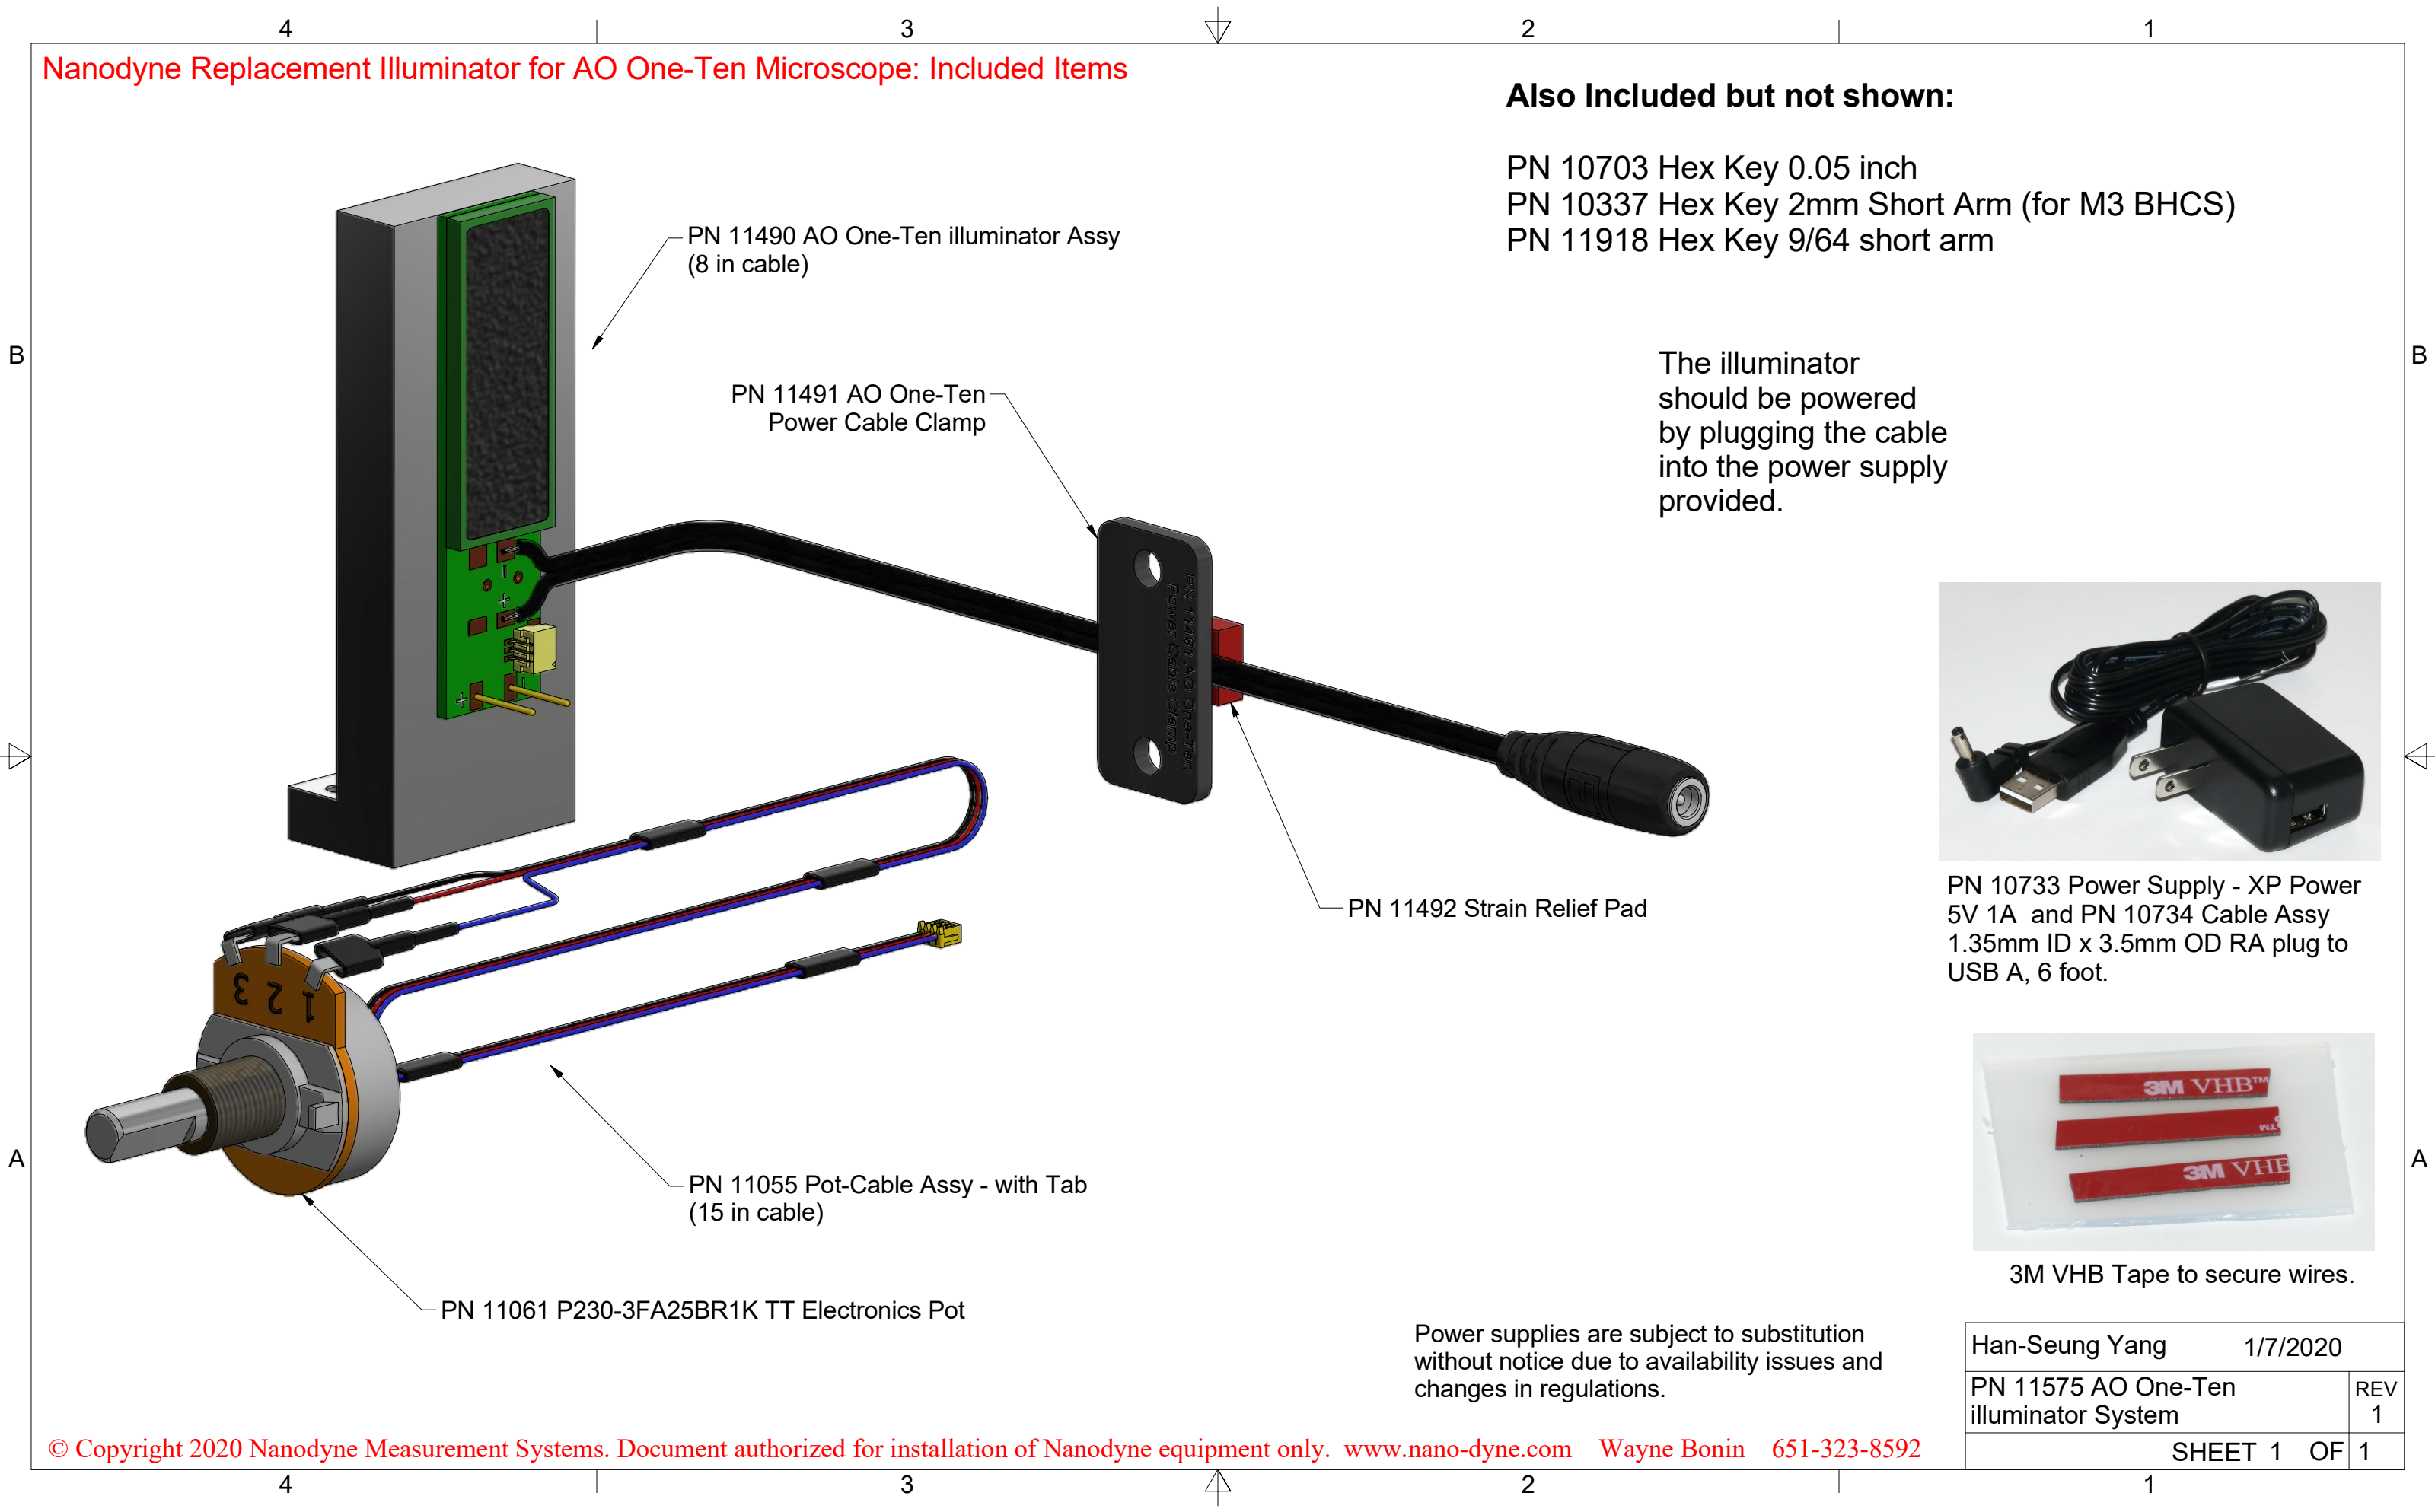

PN 10733 Power Supply - XP Power 5V 1A and PN 10734 Cable Assy 1.35mm ID x 3.5mm OD RA plug to USB A, 6 foot.



3M VHB Tape to secure wires.

Power supplies are subject to substitution without notice due to availability issues and changes in regulations.

Han-Seung Yang	1/7/2020	
PN 11575 AO One-Ten illuminator System		REV 1
SHEET 1 OF 1		