


Nanodyne Replacement Illuminator for Olympus CH Microscope - Included Items

Additional Items Included But Not Shown:

- PN 10337 Hex Key 2mm (for 3mm (M3) screws)
- PN 10747 Hex Key 3mm (for 4mm screws holding microscope base in place)
- PN 10460 Hex Key 4mm (for 6mm (M6) screw)

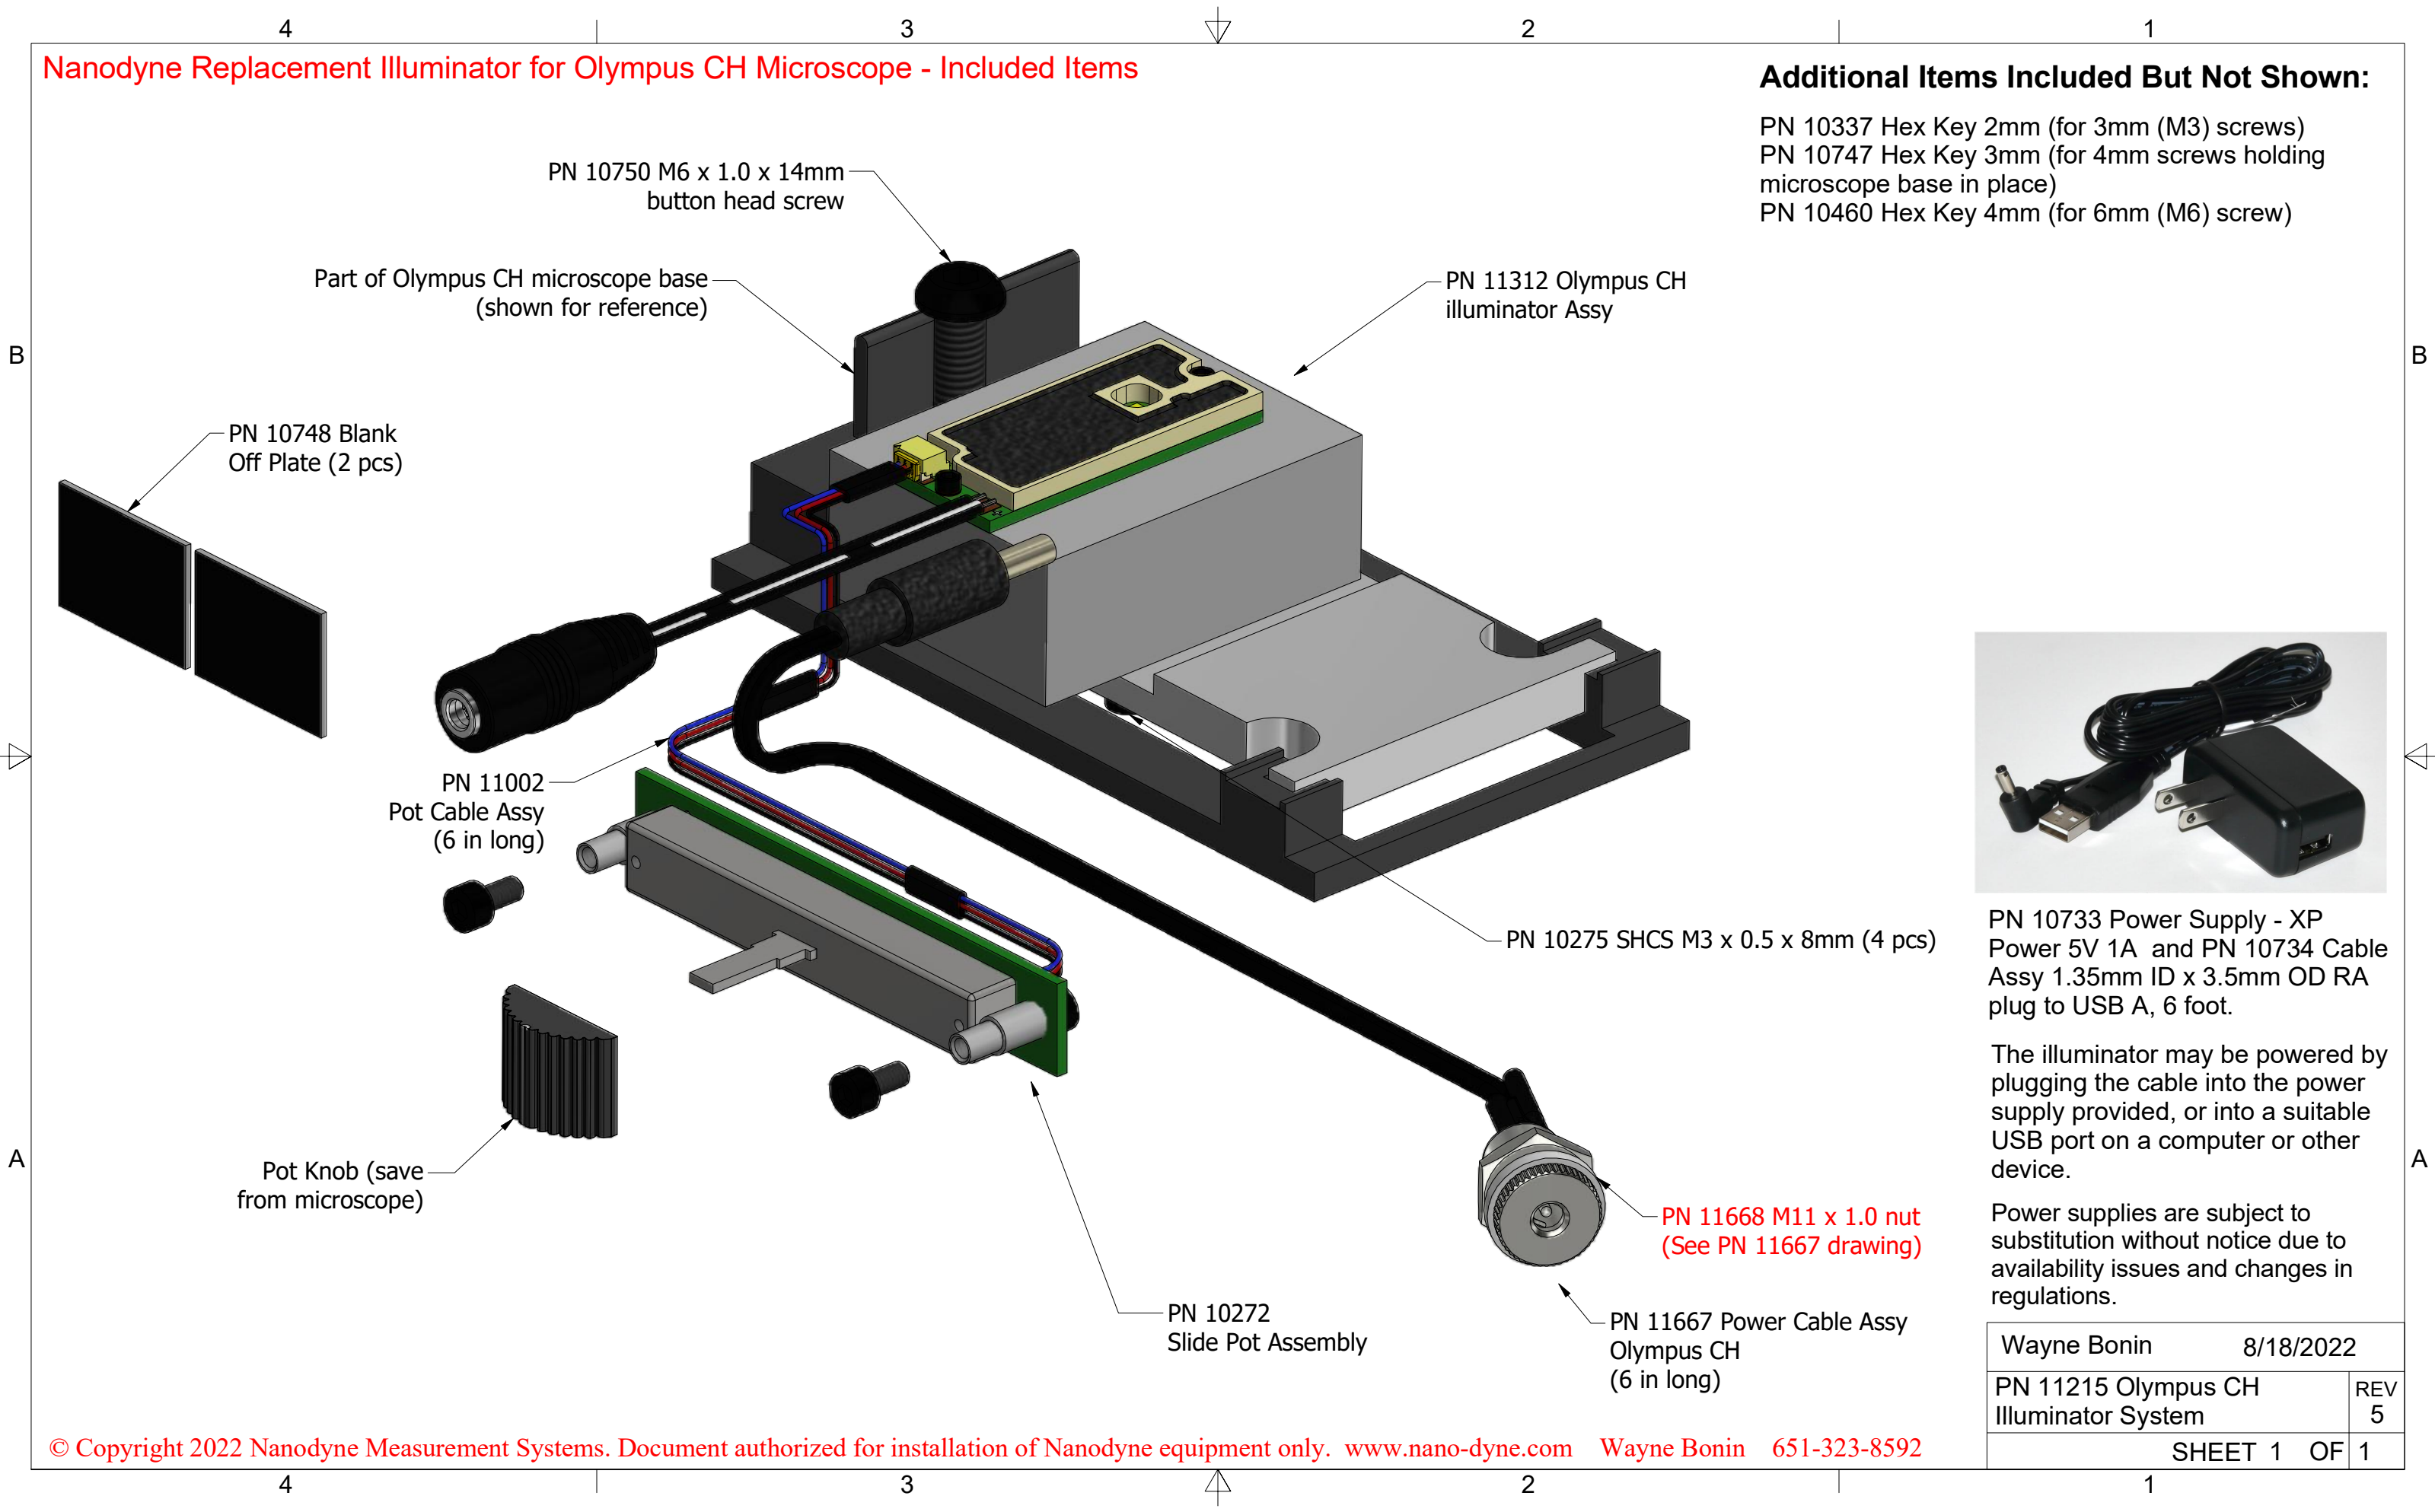

PN 10733 Power Supply - XP Power 5V 1A and PN 10734 Cable Assy 1.35mm ID x 3.5mm OD RA plug to USB A, 6 foot.

The illuminator may be powered by plugging the cable into the power supply provided, or into a suitable USB port on a computer or other device.

Power supplies are subject to substitution without notice due to availability issues and changes in regulations.

Wayne Bonin 8/18/2022	
PN 11215 Olympus CH Illuminator System	REV 5
SHEET 1 OF 1	